


SteriCheck®

Closed Sterility Test System

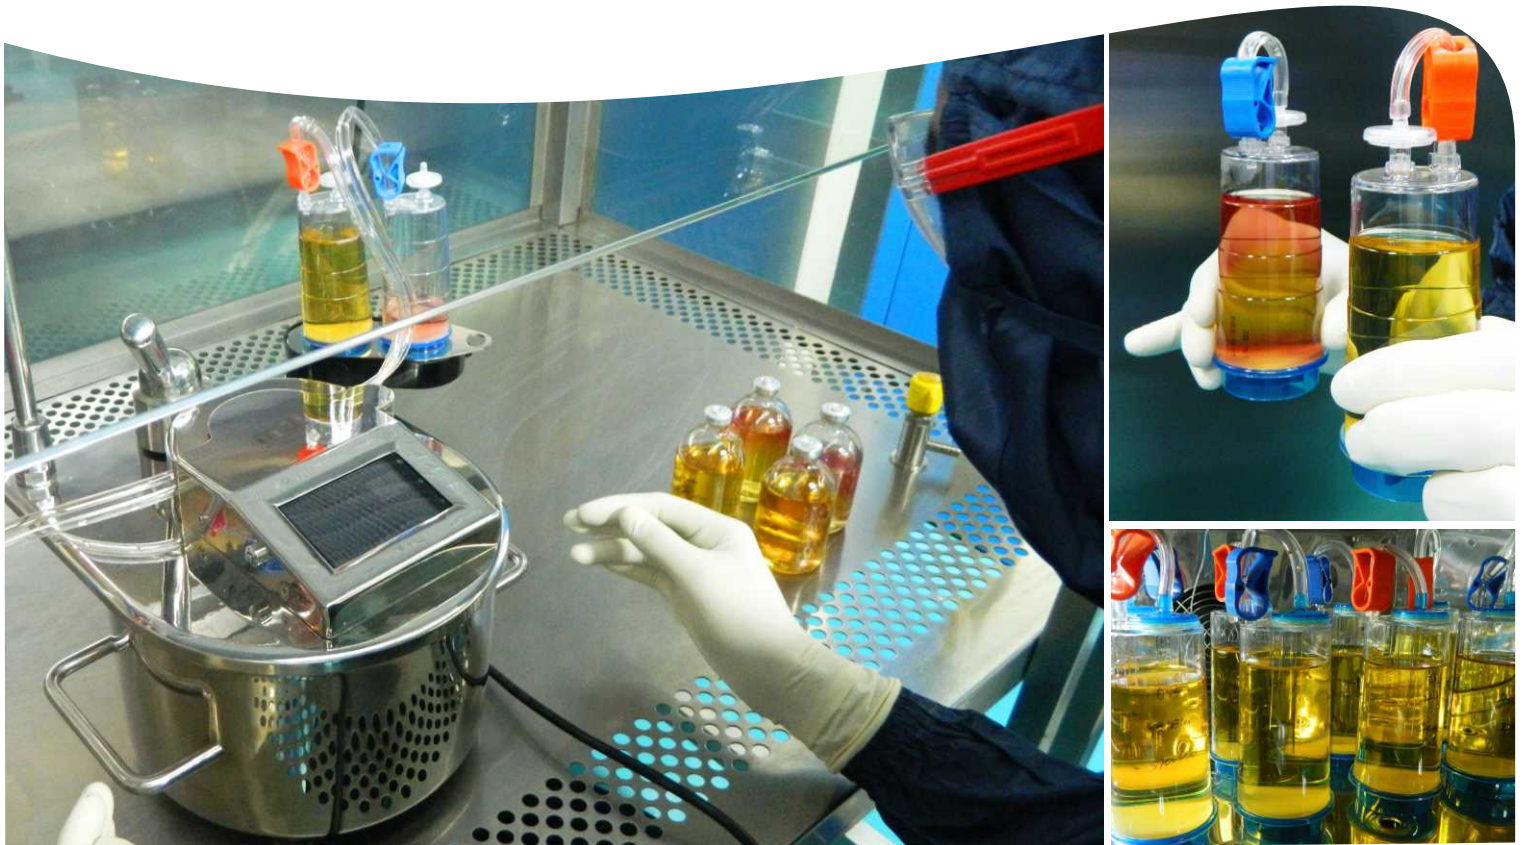

- Minimizes risk of false positives/negatives
- Meets global regulatory requirements

mdi
Membrane Technologies

SteriCheck®

Sterility Test Devices



Pre-sterilized, Ready to use


- Gamma irradiated
- EO Sterilized

Validated for

- Sterility
- Microbial Recovery
- Microbial Retention
- Equal Sample Distribution



Unique Performance Advantage

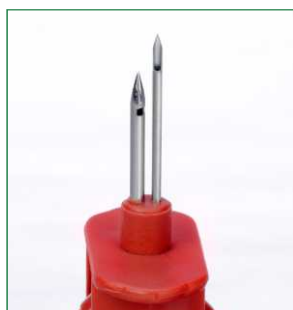

Non Coring Needle Design

- To prevent blockage by rubber particles from vial bungs

Pre-installed Color Coded Clamps

- For easy identification and clamping at both ends of the tube





Raised Transparent Vent

- To minimize chances of fluid logging and subsequent obstruction of air flow
- For easy visibility in case of accidental fluid logging

Special 'L' shaped Flow Directors

- To minimize frothing, specially with viscous fluids



Tough Membrane

- Withstands inadvertent back pressure
- Available with three different polymeric tough membranes

Archivable Chemical Indicator

- In each Stericheck pack as evidence of EO gas sterilization



Easy to Peel off, Impervious Blister Pack Cover

- For radiation sterilized Stericheck devices to prevent ingress of H_2O_2 during isolator disinfection

Customized Needle Connections


- For specific customer needs such as mini vials and cartridges in biopharmaceuticals



Applications


SteriCheck® SVP1

Small Volume Parenterals
Liquid Vials




SteriCheck® SVP2

Ampules & Collapsible bags




SteriCheck® SVP3

Small Volume Parenterals
Vials with soluble powder




SteriCheck® SVP4

Small Volume Parenterals
Mini Vials and Cartridges




SteriCheck® PC

Plastic containers




SteriCheck® LVP

Large Volume Parenterals
in glass bottles




SteriCheck® MPFS

Medical devices with
Male Luer Connection




SteriCheck® ML

Medical devices with
Female Luer Connection




SteriCheck® PFS

Pre-filled Syringes



SVP Dilutor

Antibiotics and difficult
to dissolve powders



Ordering Information

For SteriCheck Canisters:

Type	Type		
	Code		
	PVDF	Cellulose Nitrate	Nylon 66*
SteriCheck® SVP1	SV1V	SV1C	SV1N
SteriCheck® SVP2	SV2V	SV2C	SV2N
SteriCheck® SVP3	SV3V	SV3C	SV3N
SteriCheck® SVP4	SV4V	SV4C	SV4N
SteriCheck® LVP	SLVV	SLVC	SLVN
SteriCheck® PC	SPCV	SPCC	SPCN
SteriCheck® PFS	SPFV	SPFC	SPFN
SteriCheck® MPFS	SMPV	SMPC	SMPN
SteriCheck® ML	SMLV	SMLC	SMLN

Size		Pore Size		XX	XX	Sterilization		Pack Size	
	Code		Code				Code		Code
47mm	09	0.45µm	02			EO Sterile	2	10	02
						Gamma Sterile	3		

*SteriCheck® Devices with Nylon 66 membrane are available as EO sterilized only

Example:

SV1C	09	02	XX	XX	2	02
------	----	----	----	----	---	----

For SVP Dilutor pack of 20: EO Sterilized: SVPDXXXXXXXXX209

Gamma Sterilized: SVPDXXXXXXXXX309

mdi Membrane Technologies INC.

75 Uteley Drive STE 103, Camp Hill, PA 17011
Phone: +1-717-412-0943, Fax: +1-717-695-9637
E-mail: rs@mdimembranetech.com
Website: www.mdimembranetech.com

ADVANCED MICRODEVICES PVT. LTD.

20-21, Industrial Area, Ambala Cantt- 133 006, India
Tel: +91 - 171-2699290, 2699471
E-mail: info@mdimembrane.com
Website: www.mdimembrane.com