

# AseptiMix™ VB

## Vented Bottle Mixer Assemblies

**mdi AseptiMix™ VB** are gamma sterilized vented bottle mixer assemblies, suitable for mixing, safe transfer and storage of biopharmaceutical products and reagents. The assembly does not require any additional hardware and can directly be placed on a magnetic mixer for mixing with a stir bar or impeller placed inside.

The stir bar/impeller inside the mixer assembly has wide chemical compatibility and it ensures the proper mixing of solution without any particle shedding.

These assemblies are fitted with a self supporting light weight, sterilizing grade 0.2µm PVDF vent filter to prevent ingress of microorganisms during filling and removal of high value products.

### Applications

- Mixing, storage and transfer of cell culture media and buffers

### Specifications

#### Materials of Construction

<b>Bottle</b>	LDPE
	PETG
<b>Cap</b>	Polypropylene
<b>Inlet Tube</b>	Platinum Cured Silicone
<b>Dip Tube</b>	Platinum Cured Silicone
<b>Vent Filter Membrane</b>	0.2 µm Hydrophobic PVDF
<b>Vent Filter Body</b>	Polypropylene
<b>Stir Bar</b>	PVDF
<b>Impeller</b>	Polypropylene

#### Toxicity

Passes Bioreactivity test, *In Vivo*, as per USP <88> for Class VI plastics

#### Endotoxin Testing

Aqueous extracts exhibit <0.25 EU/ml as established by Limulus Amebocyte Lysate (LAL) Test as per USP <85>

#### Extractables

Passes NVR test as per USP <661>

#### Fiber Release

Passes test as per USP and comply with USFDA Title 21 CFR Part 210.3(b)(6) for fiber release

#### Particle Release

Complies with USP <788> test for particulate matter in injections



with Stir Bar



with Impeller

### Sterility Assurance

**mdi AseptiMix™ VB** vented bottle mixer assemblies are sterilized by gamma irradiation to provide a sterility assurance level of  $10^{-6}$ . The sterilization process has been validated as per ISO 11137-2 which includes dose verification, dose mapping and quarterly dose audits.

The sterilization dose of 25 kGy has been substantiated through careful definition of the test samples, bio-burden testing of multiple lots of the selected test samples, calculation of verification dose and sterility testing.


## Quality Management System

**mdi** AseptiMix™ VB vented bottle mixer assemblies are well designed products with in-built quality assurance. ISO-9001:2015 Certified Quality Management System, careful selection of raw materials, validated production processes and testing procedures based on international standards and guidelines such as CFR, PDA, and ASTM, ensures manufacture of consistently high quality assemblies.

## Customization

**mdi** AseptiMix™ VB vented bottle mixer assemblies can be customized to suit user requirements in terms of tubing, fittings, end connections and connectors.

## Product Realization Flow Chart

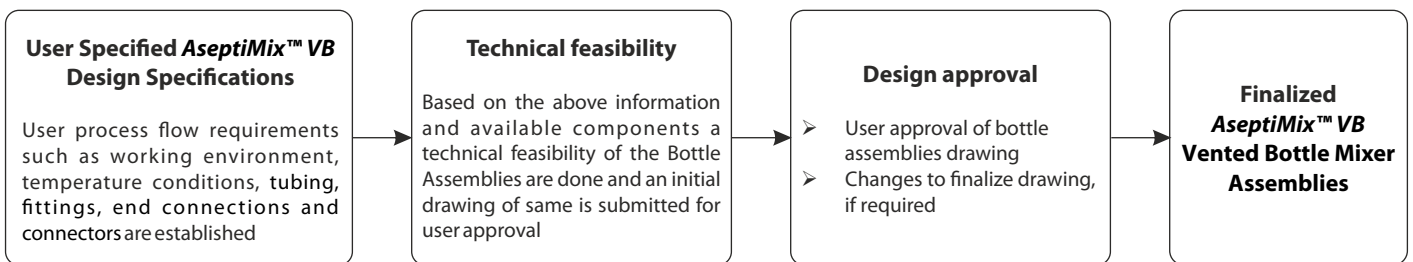

## Manufacturing Facilities

These bottle mixer assemblies are manufactured in clean rooms certified by external agencies and monitored in-house for viable and non viable particles. Employee hygiene, change rooms, gowning and de-gowning procedures and continuous monitoring of the areas is an essential part of these facilities. These facilities have been designed for unidirectional work flow with appropriate change rooms for personnel and pass boxes for material movement.

## **mdi** Membrane Technologies INC.

75 Utley Drive STE 103, Camp Hill, PA 17011  
Phone: +1-717-412-0943, Fax: +1-717-695-9637  
E-mail: rs@mdimembranetech.com  
Website: www.mdimembranetech.com

## **ADVANCED MICRODEVICES PVT. LTD.**

20-21, Industrial Area, Ambala Cantt- 133 006, India  
Tel: +91 - 171-2699290, 2699471  
E-mail: info@mdimembrane.com  
Website: www.mdimembrane.com